

For Veterinary Use Only

READ ALL INSTRUCTIONS BEFORE BEGINNING THE TEST

 RIDX™ CDV Ag Test Kit

[Catalogue Number: CGM-CDG-11, CGM-CDG-12]

Introduction

Canine distemper is highly contagious and fatal disease of dogs with a worldwide distribution. Canine distemper virus (CDV, the species *Canine morbillivirus*), an enveloped, negative-sense, single-stranded RNA virus, is a member of the genus *Morbillivirus* in the family Paramyxoviridae^{1,2}.

CDV infects different cell types, including epithelial, mesenchymal, neuroendocrine and hematopoietic cells of various organs and tissues³. A diphasic fever is a characteristic feature of the disease, occurring 7 or 8 days after infection, that drops rapidly and again climbs by day 11 or 12^{4,5}. Clinical signs of distemper are often unapparent or initially mild during this time, and the disease is characterized by mucopurulent oculonasal discharges, conjunctivitis, respiratory distress, anorexia, vomiting, diarrhea and dehydration, and cutaneous rash. Additional clinical signs that may occur are localized twitching, ascending paresis/paralysis, and/or convulsions. Hyperkeratosis of the foot pads and nose also may occur. Dogs that recover from acute disease with persistent infection may shed virus in urine and through the skin on the foot pads^{4,5}.

Domestic dogs are the main host for CDV and could also be considered as a reservoir for other mammals. Due to its high morbidity and mortality rates and broad host range, CDV is not only a well-known pathogen of domestic dogs but also one of the most important pathogens of mammals with the ability to jump the species barrier and perhaps even infect humans⁶.

Principle

The RIDX™ CDV Ag Test Kit is a lateral flow chromatographic immunoassay for the qualitative detection of CDV antigens in canine eye discharges. This kit shows two lines which are the test (T) line and the control (C) line on the surface of the device. If the CDV antigen exists in the sample, it binds to the gold-conjugated anti-CDV antibody. The antigen-antibody complex moves through the membrane by capillary force and responds to the anti-CDV antibody on the test line, resulting in a red line. The control line indicates that the test is performed correctly and should appear when the test is complete.

The highly selective and sensitive monoclonal antibody to CDV is used as a capture and detector in the kit. The RIDX™ CDV Ag Test Kit can detect CDV in canine eye discharge (conjunctiva) with high accuracy.

Performance

1. Sensitivity & Specificity

		RT-PCR		
		+	-	Total
RIDX™	+	85	3	88
CDV Ag	-	1	129	130
Test	Total	86	132	218

Sensitivity: 98.84% (85/86, *95% CI: 93.70% ~ 99.79%)

Specificity: 97.73% (129/132, 95% CI: 93.53% ~ 99.22%)

Diagnostic Agreement: 98.17% (214/218, 95% CI: 95.38% ~ 99.28%)

* 95% CI: 95% Confidence Interval

2. Limit of Detection: 5×10^3 TCID₅₀/mL

3. Cross-Reactivity

Potentially cross-reactive substances listed below have no effect on the performance of the RIDX™ CDV Ag Test Kit.

Pathogen	Titer	Result
Canine coronavirus	1.00×10^6 TCID ₅₀ /mL	Negative
Canine influenza virus	1.00×10^6 EID ₅₀ /mL	Negative
Canine parvovirus	1.00×10^6 TCID ₅₀ /mL	Negative
<i>Escherichia coli</i>	3.56×10^8 CFU/mL	Negative
<i>Giardia</i> spp.	1.42×10^5 Cysts/ μ L	Negative
<i>Salmonella</i> spp.	1.00×10^6 CFU/mL	Negative

Kit Components

Component	Quantity/kit by CAT No.	
	CGM-CDG-11	CGM-CDG-12
1 CDV Ag test device	10	2
2 Sample dilution buffer	10	2
3 Disposable swab	10	2
4 Disposable dropper	10	2
5 Instructions for use	1	1

Storage & Stability


1. Store the test kit at 2~30°C (35.6~86.0°F). **Do not freeze.**
2. Do not store the test kit in direct sunlight.
3. The test kit is stable within the expiration date marked on the package label.

Sample Preparation

1. **Canine conjunctival (eye discharges) swab** should be used as the specimen for this test kit.
2. The samples should be tested **immediately** after collection.
3. If samples cannot be tested immediately, they should be stored at 2~8°C (35.6~46.4°F) for up to 24 hours. For longer storage, freeze at -20°C (-4°F) or below. But, results from samples frozen for over one month may differ from those obtained before freezing. Frozen samples should be brought to room temperature (15~30°C/59~86°F) before use.

Test Procedure

1. All reagents must be at room temperature (15~30°C/59~86°F).
2. Collect eye discharge sample using a swab.
3. Put the swab into the sample dilution buffer and stir the solution with the swab to disperse the sample into the buffer (approximately 10 seconds).
4. Remove the swab from the sample dilution buffer.
5. Wait for 20 seconds to settle down the large particles.
6. Remove the test device from the pouch and place it on a flat and dry surface.
7. Take the supernatant sample in the tube by using a disposable dropper.
8. Apply 4 drops of the mixed sample into the sample hole (S), drop by drop vertically.
9. Read test result at 10 minutes. **Do not read results after 10 minutes.**

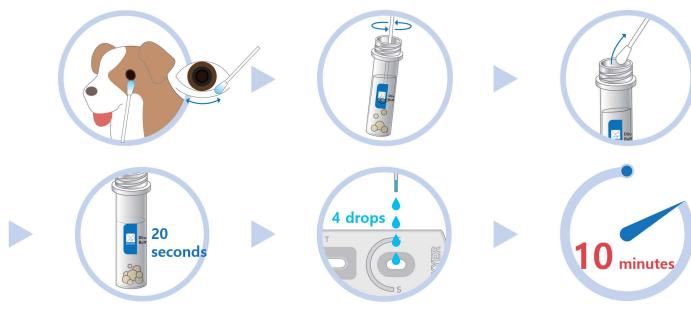

[Summary of Test Procedure]

◆ Interpretation of Results

1. Positive result

Test (T) line and control (C) line within the result window indicate the presence of CDV antigens.



2. Negative result

Only control (C) line appears in the result window.



3. Invalid results

If the control (C) line does not appear, the result might be considered invalid. The sample should be retested.



◆ Precautions

1. This test kit is for veterinary *in vitro* diagnostic use only for dogs. Do not use this test kit for other animals.
2. This rapid kit is only for preliminary screening. The final decision should be made by a qualified veterinarian based on the results of this kit, clinical symptoms and evaluation by a veterinarian, and, if necessary, the results of additional detailed diagnostic procedures.
3. The test device is sensitive to humidity and heat. Use the test device within 10 minutes after removing the foil pouch.
4. Do not touch the membrane of the test device.
5. The device should not be used if the foil pouch is damaged or has been stored with the seal open.
6. Do not use an expired test kit. The expiration date is marked on the package label.
7. Do not reuse the components (device, buffer, dropper, and swab).
8. Do not mix components from different lot numbers because the components in this kit have been quality control tested as a standard batch unit.
9. Decontaminate and dispose of all samples, used kits, and potentially contaminated materials in the accordance with national and local regulations.
10. All samples should be handled as being potentially infectious. Wear protective gloves while handling samples. Wash hands thoroughly afterward.

◆ References

1. International Committee on Taxonomy of Viruses (ICTV). *Virus Taxonomy*. 2019 Release. Ratification March 2020 (Master Species List

#35). <https://talk.ictvonline.org/taxonomy>

2. Rendon-Marin S, Budaszewski RF, Canal CW, Ruiz-Saenz J. Tropism and molecular pathogenesis of canine distemper virus. *Virol J*. 2019; 16: 30.
3. Beineke A, Puff C, Seehusen F, Baumgärtner W. Pathogenesis and immunopathology of systemic and nervous canine distemper. *Vet Immunol Immunopathol*. 2009; 127(1-2): 1-18.
4. Deem SL, Spelman LH, Yates RA, Montali RJ. Canine distemper in terrestrial carnivores: a review. *J Zoo Wildl Med*. 2000; 31(4): 441-451.
5. Kapil S, Yeary TJ. Canine Distemper Spillover in Domestic Dogs from Urban Wildlife. *Vet Clin Small Anim*. 2011; 41: 1069-1086.
6. Duque-Valencia J, Sarute N, Olarte-Castillo XA, Ruiz-Sáenz J. Evolution and Interspecies Transmission of Canine Distemper Virus-An Outlook of the Diverse Evolutionary Landscapes of a Multi-Host Virus. *Viruses*. 2019; 11(7): 582.

◆ Symbol Descriptions

	License number
	Catalogue number
	Batch code, Lot number
	Consult instructions for use
	Contains sufficient for $\langle n \rangle$ tests
	Do not reuse
	<i>In vitro</i> diagnostic medical device
	Temperature limitation
	Do not use, if the package is damaged
	Upper side
	Manufacturer



SKYER, INC.

#532, 416, Hwagok-ro, Gangseo-gu, Seoul, 07548,
Republic of Korea
TEL: +82-2-706-6801, FAX: +82-50-4096-6988
Technical Support: marketing@skyer.co.kr
www.skyerdiagnostics.com

Korean Veterinary Diagnostics Manufacturer License No. 300